

Manual Control for Driving an Intelligent Wheelchair: A Comparative Study of Joystick Mapping Methods*

Brígida Mónica Faria, Luís Ferreira, Luís Paulo Reis, Nuno Lau, Marcelo Petry, and João Couto Soares

Abstract — Electric wheelchairs are now more intelligent due to the use of algorithms that provide assisted driving. Typically, the user steers the electric wheelchairs with conventional analog joysticks. This implies the need for an appropriate methodology to map the position of the joystick handle in a Cartesian coordinate system to the wheelchair motor velocities. This mapping of joystick positions to individual wheel speed can be done in an infinite number of combinations. However it is this mapping that will determine the response behavior of the wheelchair to the user manual control. This paper describes the implementation of several joystick mappings in an intelligent wheelchair prototype. Experiments were performed in a realistic simulator using 25 users with distinct driving abilities. The users had 6 different joystick control mapping methods and for each user the usability and preference order was measured. The results achieved enable to conclude that a more direct mapping between the joystick's coordinates and the wheelchair behavior is preferred by the majority of the users.

I. INTRODUCTION

Nowadays the scientific community gives high importance to the real application of the new discoveries. In the area of assistive technologies the robotics performs an important role. In particular, electric wheelchairs are now more intelligent due the implementation of algorithms that assists the user driving.

*Research supported by ERDF – European Regional Development Fund through the COMPETE Programme (operational programme for competitiveness) and by National Funds through FCT - Portuguese Foundation for Science and Technology within project «INTELLWHEELS - Intelligent Wheelchair with Flexible Multimodal Interface, RIPD/ADA/109636/2009».

B. M. Faria is with the ESTSP/IPP - Escola Superior de Tecnologia da Saúde do Porto/Instituto Politécnico do Porto, with the DETI/UA - Departamento Electrónica, Telecomunicações e Informática, IEETA - Instituto de Engenharia Electrónica e Telemática de Aveiro, Portugal and with the LIACC - Laboratório de Inteligência Artificial e Ciência de Computadores, Universidade do Porto, Portugal (corresponding author e-mail: btf@estsp.ipp.pt).

L. Ferreira, is with IEETA – Instituto de Engenharia Electrónica e Telemática de Aveiro, Portugal (e-mail: luismferreira@ua.pt).

L. P. Reis is with the LIACC - Laboratório de Inteligência Artificial e Ciência de Computadores, Universidade do Porto, Portugal and with the EEUM - Escola de Engenharia da Universidade do Minho, Departamento de Sistemas de Informação, Portugal (e-mail: lpreis@dsi.uminho.pt).

N. Lau, is with DETI/UA - Departamento Electrónica, Telecomunicações e Informática and IEETA – Instituto de Engenharia Electrónica e Telemática de Aveiro, Portugal (e-mail: nunolau@ua.pt).

M. Petry is with the INESC TEC - Instituto de Engenharia de Sistemas e Computadores Tecnologia e Ciência, Universidade do Porto, Portugal (e-mail: (marcelo.petry@fe.up.pt).

J. C. Soares is with the LIACC - Laboratório de Inteligência Artificial e Ciência de Computadores, Universidade do Porto, Portugal (e-mail: joao.couto.soares@fe.up.pt).

Normally electric wheelchairs are manually steered with a joystick, although there are several other possibilities for the interface between a user and the wheelchair [1-4]. A conventional joystick maps the position of the handle in a Cartesian coordinate system where normalized axis (x, y) range from minus one to plus one and coordinates at the origin correspond to the central (resting) position.

An electric wheelchair is typically driven by two individually powered wheels which rotate around the horizontal axis, and another two non-powered wheels which besides rotating around a horizontal axis, also have the ability to rotate around a vertical axis. This vertical rotation axis allows the non-powered wheels to steer freely, minimizing friction during direction change. Assuming the terrain is flat and there are no obstacles, when the speed is the same on both wheels, the wheelchair moves in a straight line. Steering is determined by the velocity difference of the powered wheels, i.e. the wheelchair will rotate towards the slower wheel, and rotate around itself when the wheels rotate in opposite directions. The radius of curvature of the wheelchair is proportional to the wheel spacing and also to the traveled distances of each wheel.

The mapping of joystick positions to individual wheel speed can be done in an infinite number of combinations, and it is this mapping that will determine the response behavior to manual control. Several of these mappings were implemented, out of which a few were selected for inclusion in this article. The level of satisfaction of the volunteers that tested different joystick mappings was measured and some interesting conclusions about mapping were achieved based on the users' feedback.

This paper is organized in six sections. The first section is composed by this introduction. The second section reports the related work and related issues that are under study. The third section briefly presents our project and solutions. The implementation of the proposed algorithms is described in section four. Next it is presented the experimental work and results. Finally some conclusions and directions for future work conclude the paper.

II. RELATED WORK

There are a significant number of scientific works related to robotic wheelchairs or intelligent/smart wheelchairs [5][6]. The study about the joystick mapping is also an issue of investigation. The authors of the work presented in [7] describe a more intuitive human interface by changing the prior mapping method of the joystick, which considers the consecutive operations of a motor of a wheelchair, to a new mapping method that corresponds to the internal model of a human being. They divided the existing joystick mapping

method into two degrees of freedom, one in the vertical axis that can control the velocity and the other, in the horizontal axis for direction control, and controlled the wheelchair with an electromyography (EMG) signal. Dicianno et al. [8] concluded that individually customized isometric devices may be superior to commercially available proportional control for individuals with tremor, even though the used filtering did not improve the wheelchair driving as expected. In [9] an evaluation of the use of force feedback joysticks with a powered wheelchair is performed and concluded that on people without disabilities there were some advantages (less collisions). Niitsuma et al. [10] introduced a vibrotactile interface that could be controlled by users even if they had not used one before, and although through the experiments for the vibration stimuli, users could not detect exact orientation of obstacles, it was possible to detect a direction of the obstacle movement. In [11] a reactive shared control system was presented which allows a semi-autonomous navigation in unknown and dynamic environments using joystick or voice commands.

III. INTELLWHEELS PROJECT

The IntellWheels project aims at developing an intelligent wheelchair platform that may be easily adapted to any commercial wheelchair and aid any person with special mobility needs [12]. The project main focus is the research and design of a multi-agent platform, enabling easy integration of different sensors, actuators, devices for extended interaction with the user, navigation methods and planning techniques and methodologies for intelligent cooperation to solve problems associated with intelligent wheelchairs [13] [14].

A real prototype (Fig. 1) was created by adapting a typical electric wheelchair. Two side bars with a total of 16 sonars, a laser range finder and two encoders were incorporated.



Figure 1. The real prototype of the IW

In order to test the algorithms and methodologies a simulator was also developed. With this simulator a virtual world can be created where a user can drive the IW with a similar behavior of the real prototype. The virtual wheelchair (Fig. 2) was modeled with the 3D Studio Max [15], the virtual environment was modeled with 3D UnrealEditor and USARSim [16] was the platform chosen for the simulation of robots and environments. USARSim is based on the Unreal Tournament game engine [16] and is intended as a general

purpose research tool with various applications from human computer interfaces to behavior generation for groups of heterogeneous robots [16].



Figure 2. The virtual prototype of the IW

The purpose of this simulator is essentially to support the testing of algorithms, analyze and test the modules of the platform and safely train users of the IW in a simulated environment [17] [18].

A multimodal interface was also developed that allows driving the wheelchair with several inputs such as joystick, head movements or more high level commands such as voice commands, facial expressions, and gamepad or even with a combination among them. For example it is possible to blink an eye and say “go” for the wheelchair follow a right wall [19] [20] [21].

The joystick mapping is important, because this mapping will determine the response behavior of the wheelchair to the user manual control. For that reason, different ways of mapping the joystick signal were tested. The next section presents different alternatives and considerations regarding the used mapping algorithms.

IV. IMPLEMENTATION OF JOYSTICK MAPPING ALGORITHMS

This section presents the implemented algorithms and their variants, aiming to achieve a more pleasant wheelchair driving experience. Considering that the joystick handle position is represented in a Cartesian coordinate system, with two axis, x and y , which vary between -1 and 1, and where these (x, y) coordinates can be used to determine the distance of the handle to the central (resting) position of the joystick $(0, 0)$ and an angle relating to a reference vector (which is usually $(0, 1)$). The desired speed of the left wheel (L) or the right wheel (R) is represented by normalized values (between -1 and 1). With positive values the wheels rotate forward and with negative values the wheels rotate backward.

The default mapping should meet the following conditions: θ is calculated in relation to vector $(0, 1)$; when θ is undefined, i.e when $(x, y) = (0, 0)$, both wheels will not be actuated; when $\theta = 0$, both wheels move forward at the same speed; when $\theta = \pm\pi$, both wheels move backward at the same speed; when $\theta = \pm\pi/2$, the wheels rotate in opposite directions and when $\theta = \pm\pi/4$, one of the wheels stops, and the other one rotates, making the chair turn around the stopped wheel.

A. Algorithm A - First Alternative

The first mapping algorithm proposed is very simple. The steering and power mapping is achieved through the use of both x and y in all instances and the wheelchair can rotate around itself when the joystick is pushed to the sides. Assuming that x and y are normalized and vary between -1 and 1 the system of equations can be observed in (1):

$$\begin{cases} R = y - x \\ L = y + x \end{cases} \quad (1)$$

Note that at the central position $(0, 0)$ no power is sent to the wheels. When x is near 0, and the joystick is pushed forward/backward, the speed increases proportionally to y , and the wheelchair moves forward/backward. There is no rotation because x equals zero, thus left speed and right speed are equal and proportional to y .

For all other values of x , when the joystick is pushed to either left or right, the right speed is proportional to $(y-x)$ and left speed is proportional to $(x+y)$. It is important to notice that the right speed and left speed are clipped when $(y-x)$ or $(x+y)$ are above the maximum normalized values. This implies a loss of the useable joystick area. Additionally, some filtering was added, so that minimal (x, y) variation near the axis is ignored. When the wheels rotate in opposite directions, speed is halved on both wheels.

With this algorithm, steering the wheelchair requires accurate precision. The wheel speed variations that derive from changes in joystick direction changes are quite steep, and when moving forward, little variations on the joystick horizontal axis, result in a big adjustment of the direction.

Fig. 3 represents the left and right wheel speed mapping as a function of the x and y positions of the joystick. Fifty percent of gray matches speed zero, lighter areas correspond to positive velocities, where white represents the maximum, and darker areas represent negative velocities, where black represents the maximum negative velocity. All tones in between correspond to an intermediate speed.

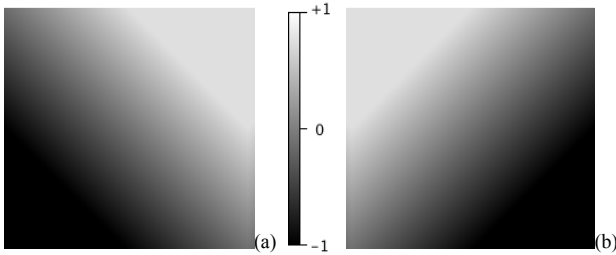


Figure 3. (a) and (b) respectively represent the left and right wheel speed mapping as a function of the x and y positions of the joystick – algorithm A.

Fig. 3 confirms that when the joystick is at $(1, 1)$, i.e. to the front and right, the left wheel speed is clipped at its maximum, and the right wheel speed is at fifty percent gray, which means the right wheel speed equals zero. In this condition, the wheelchair will rotate around the right wheel.

When the joystick is maintained at $x=1$ and y is pulled from 1 towards 0, left wheel speed is maintained and right wheel speed becomes negative, reaching the maximum

negative speed when y equals zero. Due to a constraint in the algorithm, the clipping at the maximum and minimum speed is quite strong (visible in the full white/full black areas) and results in a loss of useable joystick area.

Attenuation with an exponential function was applied to the input variables of the algorithm and Fig. 4 shows a significantly improvement in terms of range extension.

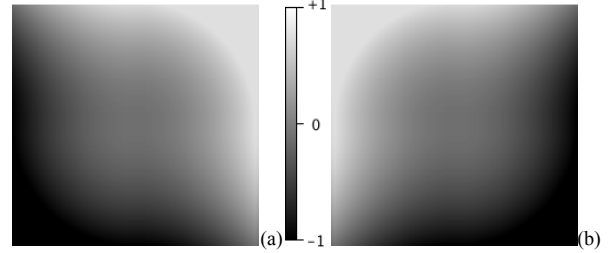


Figure 4. (a) and (b) respectively represent the left and right wheel speed mapping as a function of the x and y positions of the joystick – algorithm A with attenuation.

B. Algorithm B – Second Alternative

In this algorithm, the distance of the handle to the center of the joystick (ρ) is proportional the maximum wheel speed and the angle (θ) of the joystick relating to the vector $(0, 1)$ determines how the speed is distributed to the wheels. In order to keep ρ minor or equal to 1, the value is clipped when ρ is above one. Assuming that x and y are normalized and vary between -1 and 1, the control follows these conditions:

$$R = \begin{cases} \rho, & \text{if } -\frac{\pi}{2} \leq \theta \leq 0 \\ -\rho, & \text{if } \frac{\pi}{2} \leq \theta \leq \pi \\ \frac{\rho \cos(\theta + \pi/4)}{\cos(-\pi/4)}, & \text{if } 0 < \theta < \frac{\pi}{2} \vee -\pi < \theta < -\frac{\pi}{2} \end{cases} \quad (2)$$

$$L = \begin{cases} \rho, & \text{if } 0 \leq \theta \leq \frac{\pi}{2} \\ -\rho, & \text{if } -\pi \leq \theta \leq -\frac{\pi}{2} \\ \frac{\rho \cos(\theta - \pi/4)}{\cos(-\pi/4)}, & \text{if } -\frac{\pi}{2} < \theta < 0 \vee \frac{\pi}{2} < \theta < \pi \end{cases} \quad (3)$$

where $\rho = \sqrt{x^2 + y^2}$ and $\theta = \arctan(y/x) - \pi/2$.

Several scenarios can occur: when $0 < \theta < \pi/2$, the right wheel speed will vary between ρ and $-\rho$, and the left wheel speed will be proportional to ρ ; when $0 > \theta > -\pi/2$, the left wheel speed will vary between ρ and $-\rho$, and the right wheel speed will be proportional to ρ ; when $\pi/2 > \theta > \pi$, the left wheel speed will vary between ρ and $-\rho$, and the right wheel speed will be proportional to $-\rho$; when $-\pi/2 < \theta < -\pi$, the right wheel speed will vary between ρ and $-\rho$, and the left wheel speed will be proportional to $-\rho$ and if $\rho > 1$, ρ is clipped back to 1 or if $\rho < -1$, ρ is clipped back to -1.

As can be seen in Fig. 5 (a) and (b), the speed variation is extended towards the corners of the joystick, and clipping is

minimized when compared to the previous algorithm, however, even though experimentally, this algorithm provides a more pleasant driving experience, steering is still not as smooth as desired.

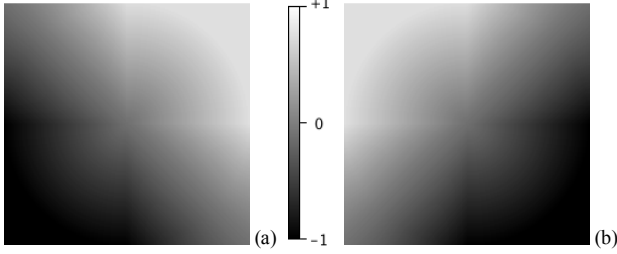


Figure 5. (a) and (b) respectively represent the left and right wheel speed mapping as a function of the x and y positions of the joystick – algorithm B.

It was also observed that as the joystick moved away from the central position, the curvature radius would decrease very fast. In order to resolve this issue, the joystick axis values were attenuated with an exponential function.

Fig. 6 (a) and (b) represent the left and right wheel speed mapping as a function of the x and y positions of the joystick, after attenuating the axis readings. Fifty percent gray matches speed zero, lighter areas correspond to positive velocities, where white represents the maximum, and darker areas represent negative velocities, where black represents the maximum negative velocity. All tones in between correspond to an intermediate speed.

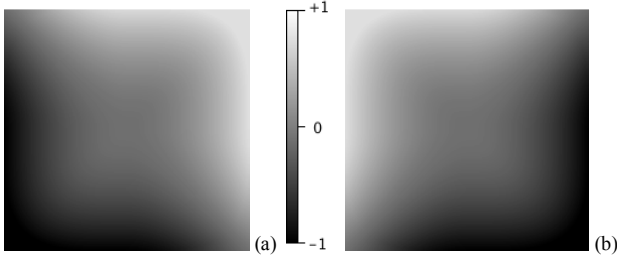


Figure 6. (a) and (b) respectively represent the Left and Right Wheel speed mapping as a function of the x and y positions of the joystick – algorithm B with attenuation.

Comparing Fig. 5 and 6, it is visible that with the input variables attenuation, the speed variation is more uniformly spread, extended towards the corners, and with minimal clipping. This attenuation can be felt while driving as a more natural, smoother and precise driving experience.

C. Algorithm C – Third Alternative

This mapping is an updated version of algorithm A. Assuming that x and y are normalized and vary between -1 and 1, the equations applied are:

$$\begin{cases} R = y - nx \\ L = y + nx \end{cases} \quad (4)$$

where the equations follow the next conditions that can be observed in the equation (5):

$$\begin{cases} \text{if } \frac{x}{2} > 0.1, & nx = 0.1 + (x/2 - 0.1)/2 \\ \text{if } \frac{x}{2} < -0.1, & nx = -0.1 + (x/2 + 0.1)/2 \\ \text{else} & nx = x/2 \end{cases} \quad (5)$$

This algorithm goes beyond the range of algorithm A, minimizing clipping as can be observed in Fig. 7.

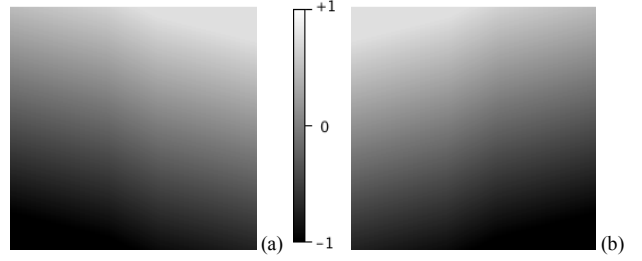


Figure 7. (a) and (b) respectively represent the Left and Right Wheel speed mapping as a function of the x and y positions of the joystick – algorithm C.

At this point, attenuation with an exponential function was also applied to algorithm C. Fig. 8 reports the difference in behavior.

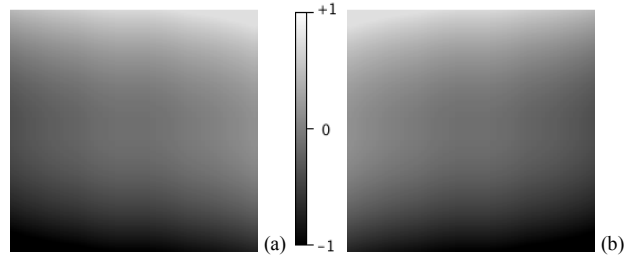


Figure 8. (a) and (b) respectively represent the Left and Right Wheel speed mapping as a function of the x and y positions of the joystick – algorithm C with attenuation.

V. EXPERIMENTS AND RESULTS

After the implementation of the control algorithms it was necessary to test with real users in order to verify the preference of the different mappings. Therefore a circuit was developed using the simulator. Fig. 9 shows the overall circuit.

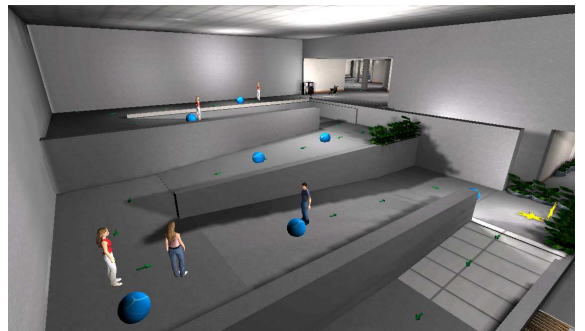


Figure 9. Circuit and taks used for testing

A kind of serious game was created. The game objective was to follow a specific track collecting eight blue balls and at the end a yellow star. The green arrows just indicate the route and the blue balls were obligatory checkpoints, since they could be collected passing near them. The people added to the environment were dynamic obstacles that should be avoided.

A quasi-experimental study was performed. The volunteers had an explanation of the purpose of the study and signed the inform consent. A questionnaire was elaborated and was composed of four parts: user identification; experience with videogames and joysticks; questions adapted from the Computer System Usability Questionnaire (CSUQ) [22] for each option tested and a final question about the preference order of the options tested. The questions from the CSUQ were measured in a Likert scale in order to obtain a final score from 0 to 100. The questions were:

- Overall, I am satisfied with how easy it is to use this control.
- It was simple to use this control.
- I can effectively complete this task using this control.
- I am able to complete this task quickly using this control.
- I am able to efficiently complete this task using this control.
- I feel comfortable using this control.
- It was easy to learn to use this control.
- Whenever I make a mistake using the control, I recover easily and quickly.
- Overall, I am satisfied with this control.

Two more specific questions were asked:

- I felt I had control of the wheelchair.
- It is easy to drive the wheelchair in narrow spaces.

All 25 individuals drove the simulated wheelchair with the six alternatives of mapping the joystick: the algorithms A, B, C and all of them with the exponential attenuation function (D, E and F respectively). The order of the experiments was randomly set to avoid the bias relative to the experience of the user. After each round the volunteers answered to several questions related to each kind of mapping.

The sample of individuals is characterized for having a mean of age of 33 years old and 4 women and 21 men. The experience with videogames and joysticks is not considerable high (Fig. 10), although there are individuals that have considerable experience with joysticks.

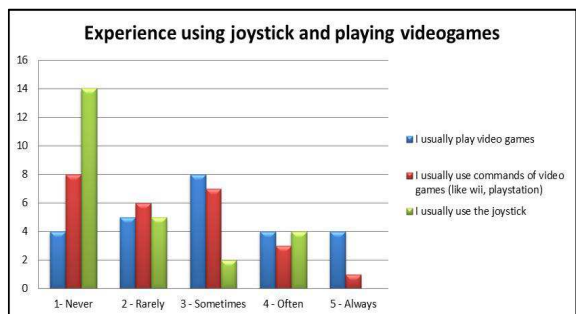


Figure 10. Responses about experience with joystick and videogames.

Table I shows the summary statistics measures about the final score for all the mapping options.

TABLE I. SUMMARY STATISTICS MEASURES OF THE ADAPTED CSUQ SCORE

Adapted CSUQ – Final Score						
Statistics	A	B	C	D	E	F
Mean	56	63,4	80,6	64,6	72,8	77,7
Median	52,4	58,7	85,7	61,9	76,2	82,5
Std. Deviation	23,6	24,6	17,4	22,7	20,0	17,5
Minimum	22,2	14,3	33,3	25,4	14,3	33,3
Maximum	100	100	100	100	95,2	98,4

The opinions about the different ways of mapping the joystick indicate that the level of satisfaction is higher when using the option C. The next option is F, then E, D, B and finally A.

To confirm that the alternatives of mapping are significantly different the statistical Friedman test (related samples Friedman's test two way analysis of variance by ranks) was applied to the final score obtained. The level of significance used was 0.05. The p value inferior of 0.001 and inferior of the level of significance allow concluding that there are statistical differences between the distributions of the scores. To identify which commands are significantly different it was necessary to use a multiple comparison of means of orders (Fisher's least significant difference (LSD)). Table II shows the p values of the multiple comparisons, using the Fisher's least significant difference (LSD).

TABLE II. MULTIPLE COMPARISONS OF THE ADAPTED CSUQ SCORE

Multiple Comparisons LSD – Adapted CSUQ Score (p values)					
	A	B	C	D	E
B	0,199	--	--	--	--
C	<0,001	<0,001	--	--	--
D	0,022	0,308	0,001	--	--
E	0,002	0,064	0,012	0,399	--
F	<0,001	<0,001	0,424	0,011	0,085

It is interesting to verify that the score of the option C is statistical different for all other options except F at a level of significance 0.05. Also there are not statistical evidences to affirm that the distribution of scores F and E are different.

The results about the score are also confirmed with the order of preference as can be observed in Table III.

TABLE III. SUMMARY STATISTICS ABOUT THE ORDER OF PREFERENCE

Order of preference (1- Best to 6- Worst)						
Statistics	A	B	C	D	E	F
Median	5	5	2	4	3	2
Minimum	1	1	1	1	1	1
Maximum	6	6	5	6	6	6

The questions about the specific behavior in the circuit suggested have their answers distribution in the Fig. 11 and Fig. 12 by each option tested.

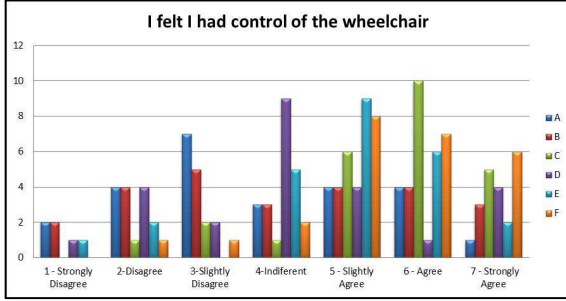


Figure 11. Responses about the feeling of control when driving the wheelchair using the different options.

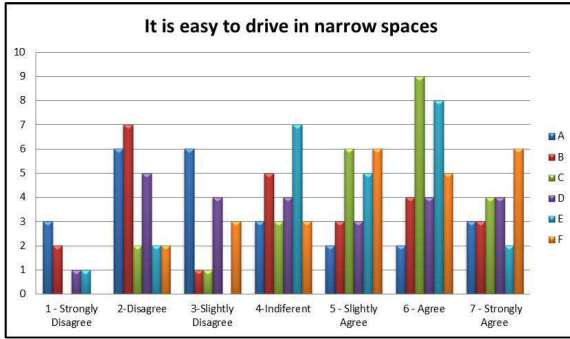


Figure 12. Responses about the experiment when driving in narrow spaces.

The feeling about control of the wheelchair is more visible using the options C and F. In terms of ease by driving the wheelchair in narrow spaces the control F had more responses as “Strongly Agree”. To confirm that the controls are significantly different the statistical Friedman test was also applied to the variables “Feeling about control of driving the wheelchair” and “easy to drive in narrow spaces”. The p values obtained were also less than 0.001, so there are statistical differences between the distribution of answers among each joystick mappings in terms of feeling about control of the wheelchair and the easily to drive in narrow spaces. The same multiple comparison of means of orders analysis was performed. Table IV and V show the corresponding p values.

TABLE IV. MULTIPLE COMPARISONS OF THE FEELING OF CONTROL OF THE WHEELCHAIR

Multiple Comparisons LSD – Feeling of control (p values)					
	A	B	C	D	E
B	0,263	--	--	--	--
C	<0,001	<0,001	--	--	--
D	0,308	0,919	<0,001	--	--
E	0,004	0,068	0,012	0,054	--
F	<0,001	<0,001	0,919	<0,001	0,009

The feeling about having control of the wheelchair with the option C and F is statistical different with all other options except with each other.

TABLE V. MULTIPLE COMPARISONS OF EASE OF DRIVING THE WHEELCHAIR IN NARROW SPACES

Multiple Comparisons LSD – Ease of driving (p values)					
	A	B	C	D	E
B	0,223	--	--	--	--
C	<0,001	<0,001	--	--	--
D	0,023	0,281	0,008	--	--
E	0,006	0,112	0,032	0,606	--
F	<0,001	0,001	0,814	0,016	0,056

The question about driving the wheelchair in narrow spaces with the six options also had p values less than 0.05. In this case the option C is also statistical different from other options except with F.

VI. CONCLUSIONS

Typically, users control electric wheelchairs using conventional analog joysticks. Thus, they need appropriate methodologies to map the position of the joystick to the wheelchair motor velocities. This paper described the implementation of several joystick mappings and appropriate experiments performed in a realistic simulator in order to analyze the usability of the joystick mapping methods.

The study conducted enabled us to verify that the intuitive mapping method achieved was preferred by the majority of the users. Using this method, users could keep the control of the Intelligent Wheelchair, even in narrow spaces.

Future work will be concerned with conducting a deeper study of the control methods by testing different configuration parameters for each control type and test the controls with broad sample of wheelchair users. Another experiment will be concerned with the use of data mining algorithms to create user driving models and using them to create automatic control methods based on real user behavior.

ACKNOWLEDGMENTS

This work was funded by the ERDF – European Regional Development Fund through the COMPETE Programme (operational programme for competitiveness) and by National Funds through FCT - Portuguese Foundation for Science and Technology within project «INTELLWHEELS - Intelligent Wheelchair with Flexible Multimodal Interface, RIPD/ADA/109636/2009». B. M. Faria thanks to FCT for the PhD Scholarship FCT/SFRH/BD/44541/2008 and M. Petry also thanks FCT for his PhD Scholarship FCT/SFRH/BD/60727/2009.

REFERENCES

- [1] S. Nakanishi, Y. Kuno, N. Shimada and Y. Shirai, “Robotic wheelchair based on observations of both user and environment,” in International Conference on Intelligent Robots and Systems, 1999.

- [2] Y. Matsumoto, T. Ino and T. Ogasawara, "Development of Intelligent Wheelchair System with Face and Gaze Based Interface," in 10th IEEE International Workshop on Robot and Human Communication, Bordeaux, 2001.
- [3] S. Ju, Y. Shin and Y. Kim, "Intelligent wheelchair (iw) interface using face and mouth recognition," in 13th international conference on Intelligent user interfaces, Canary Islands, 2009.
- [4] A. Sasou and H. Kojima, "Noise robust speech recognition applied to voice-driven wheelchair," *Journal on Advances in Signal Processing*, vol. 1, no. 41, 2009.
- [5] R. A. M. Braga, M. Petry, A. P. Moreira, L. P. Reis, Concept and Design of the Intellwheels Platform for Developing Intelligent Wheelchairs, Springer-Verlag, LNEE/ Informatics in Control, Automation and Robotics. Vol 37. April, 2009, pp. 191-203.
- [6] R. Simpson, "Smart wheelchairs: A literature review," *Journal of Rehabilitation Research & Development*, pp. 423-435, July/August 2005.
- [7] K. Choi, M. Sato and Y. Koike, A new human-centered wheelchair system controlled by the EMG signal, International Joint Conference on Neural Networks, Vancouver, BC, Canada July 16-21, 2006.
- [8] B. E. Dicianno, S. Sibenaller, C. Kimmich, R. A. Cooper, J. Pyo, Joystick use for virtual power wheelchair driving in individuals with tremor: Pilot study, *Journal Rehabilitation Research & Development*, Vol 46, No 2, 2009, pp. 269-276.
- [9] A. Fattouh , M. Sahnoun , G. Bourhis, Force Feedback Joystick Control of a Powered Wheelchair: Preliminary Study, IEEE International Conference on Systems, Man and Cybernetics, vol.3, pp. 2640 – 2645, 2004.
- [10] M. Niitsuma, T. Ochi, M.Yamaguchi, H. Hashimoto, Interaction between a User and a Smart Electric Wheelchair in Intelligent Space, International Symposium on Micro-NanoMechatronics and Human Science (MHS), Nov 2010, pp. 465-470.
- [11] G. Pires, U. Nunes, A wheelchair steered through voice commands and assisted by a reactive fuzzy-logic controller, *Journal of Intelligent and Robotics System*, 34, pp. 301-314, 2002.
- [12] R. Braga, M. Petry, L. L. Reis, A. P. Moreira, IntellWheels: Modular development platform for intelligent wheelchairs, *Journal of Rehabilitation Research & Development*, 48, 9, 2011, pp. 1061-1076.
- [13] R. Braga, M. Petry, A. P. Moreira, L. P. Reis. Intellwheels: A Development PlatForm for Intelligent Wheelchairs for Disabled People. Proceeding of the 5th International Conference on Informatics in Control, Automation and Robotics. Vol I. Funchal, Madeira, Portugal, pp.115-121, 2008.
- [14] M. Petry, A. P. Moreira, R. Braga, L. P. Reis, Shared Control for Obstacle Avoidance in Intelligent Wheelchairs, 2010 IEEE Conference on Robotics, Automation and Mechatronics (RAM 2010), June 28–30 2010, Singapore, pp. 182-187.
- [15] K. L. Murdock, 3ds Max 2011 Bible, Indianapolis: John Wiley & Sons, 2011.
- [16] S. Carpin, M. Lewis, J. Wang, S. Balakirsky and C. Scrapper, "USARSim: a robot simulator for research and education," in Proceedings of the IEEE International Conference on Robotics and Automation, Roma, Italy, 2007.
- [17] R. Braga, P. Malheiro, L. P. Reis, Development of a Realistic Simulator for Robotic Intelligent Wheelchairs in a Hospital Environment, In J.Baltes, M.Lagoudakis, T.Naruse, S.Shiry (Eds.), RoboCup 2009, LNAI 5949, pp. 23-34. Springer, Heidelberg, 2010, Graz, Austria, 2009.
- [18] M. Petry, A. P. Moreira, L. P. Reis, R. Rossetti, Intelligent Wheelchair Simulation: Requirements and Architectural Issues, in 11th International Conference on Mobile Robotics and Competitions, Lisbon, 2011.
- [19] B. M. Faria, S. Vasconcelos, L. P. Reis, N. Lau, A Methodology for Creating Intelligent Wheelchair Users' Profiles, ICAART 2012 - 4th International Conference and Artificial Intelligence, Algarve, 2012, pp 171-179.
- [20] L. P. Reis, R. Braga, M. Sousa, A. P. Moreira. Intellwheels MMI: A Flexible Interface for an Intelligent Wheelchair, RoboCup Symp2009, In J.Baltes, M.Lagoudakis, T.Naruse, S.Shiry (Eds.): RoboCup 2009, LNAI 5949, pp. 296-307. Springer, Heidelberg, 2010, Graz, Austria.
- [21] B. M. Faria, S. Vasconcelos, L. P. Reis, N. Lau, Evaluation of Distinct Input Methods of an Intelligent Wheelchair in Simulated and Real Environments: A Performance and Usability Study Assistive Technology: The Official Journal of RESNA, Accepted 05 Sep 2012.
- [22] J. R. Lewis, IBM Computer Usability Satisfaction Questionnaires: Psychometric Evaluation and Instructions for Use, International Journal of Human-Computer Interaction 7, 1, 1995, pp. 57-78.